


HPLC Conditions

Column: Discovery BIO Wide Pore C18 HPLC, 250 x 4.6 mm, 5 μ m
Mobile Phase: A. 25 mM ammonium acetate in water, pH 5
B. Acetonitrile
Gradient: 23 to 65% B in 30 minutes
Flow rate: 1 mL/min
 λ =240 nm
Sample: 0.25 mg/mL in 10% Acetonitrile/25 mM ammonium acetate, pH 5
Injected: 30 μ L

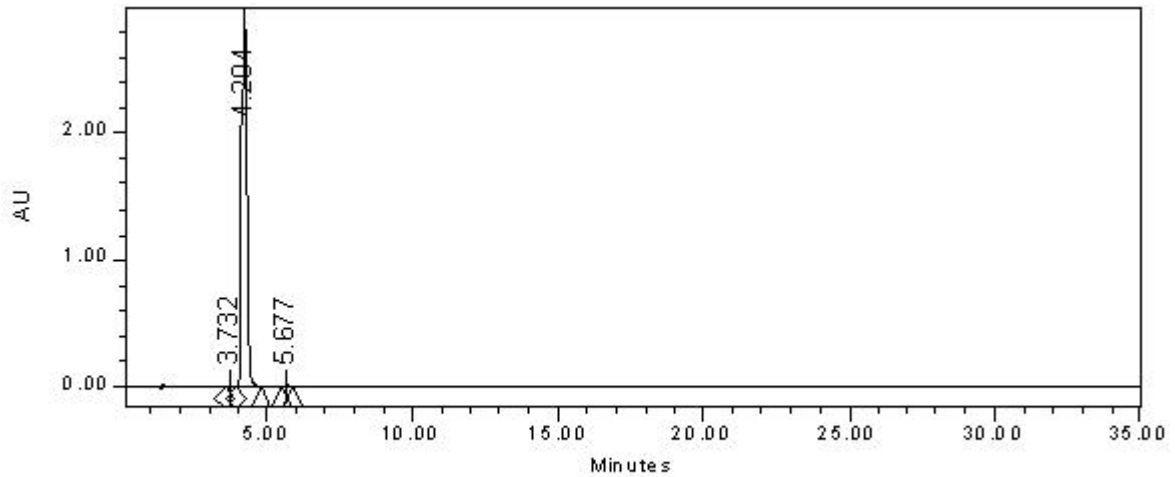

Purity

Peak	Retention Time	Area	% Area
1	3.732	94516	0.29
2	4.204	31867294	99.43
3	5.677	89021	0.28